



FORTESSA CONGIG 082514

Cytometer:	LSRFortessa	User:	BDService
Cytometer Name:	LSRFortessa	Institution:	
Serial Number:	1	Software:	BD FACSDiva 6.2
Input Device:	Manual	Date:	8/25/2014 2:37:05 PM
Window Extension:	10.00		


Blue Laser
(488nm)
FSC

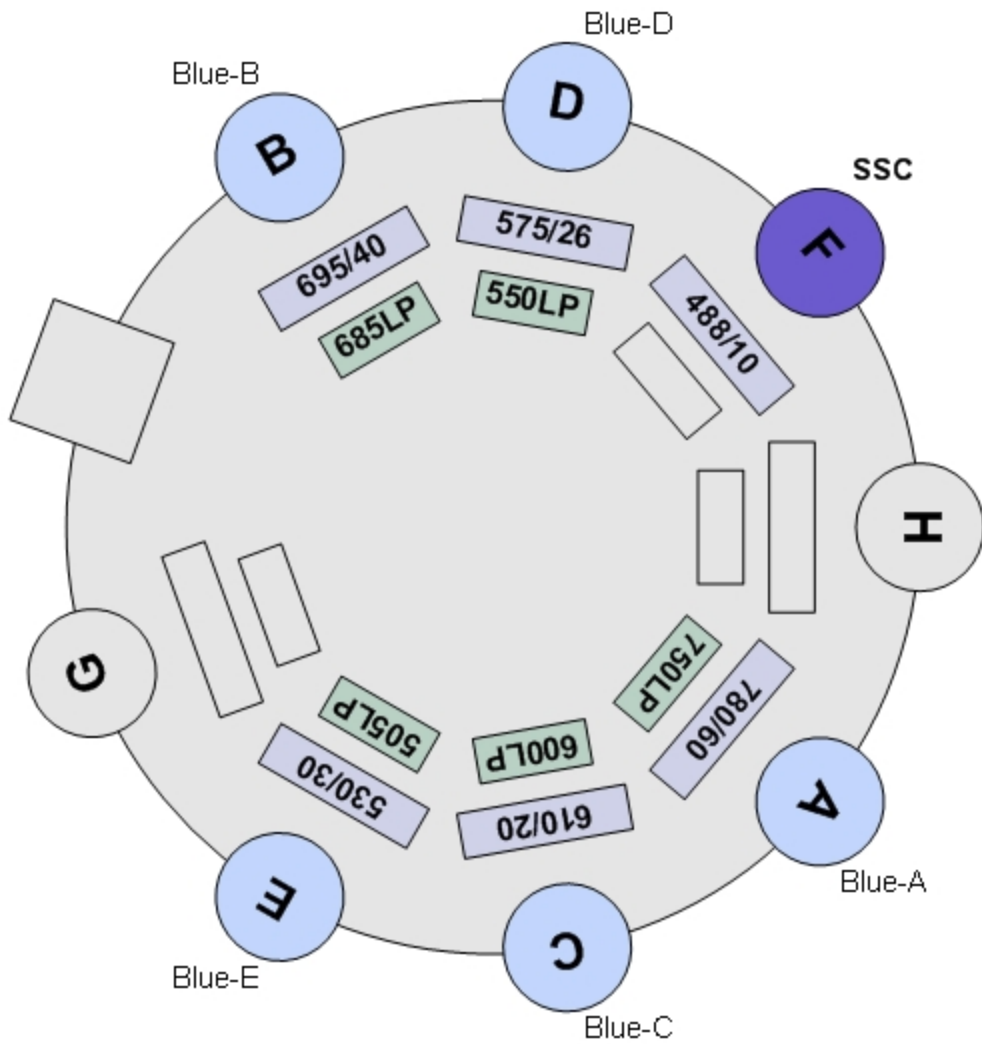

Red Laser
(640nm)

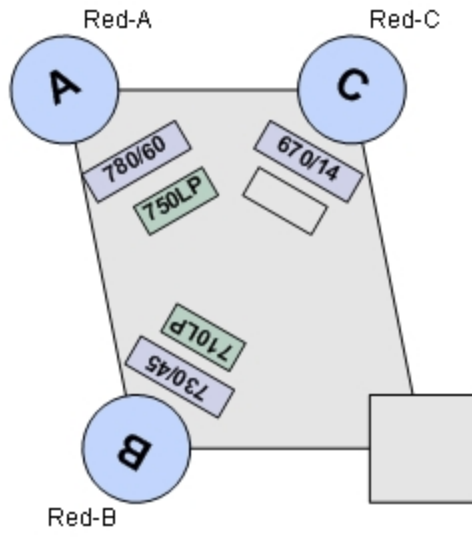

Violet Laser
(405nm)

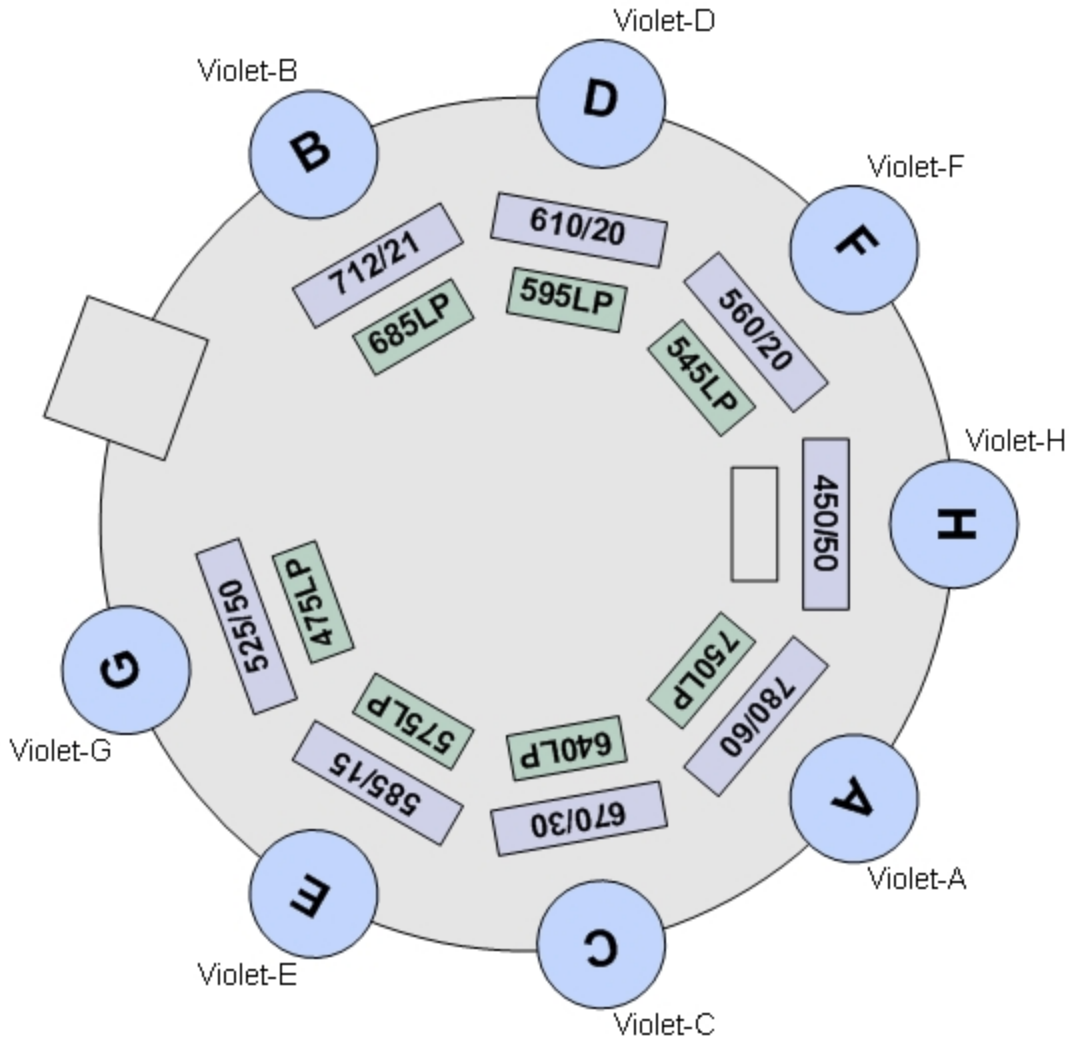

Comments: